



KYORITSU

PACKTEST

INSTRUCTIONS

Magnesium


Model WAK-Mg-2

Titan Yellow Visual Colorimetric Method

Main Reagent: Titan Yellow

Measuring Range: Mg 0 - 20mg/L (ppm)
(Hardness) CaCO₃ 0 - 82mg/L (ppm)

How to Use

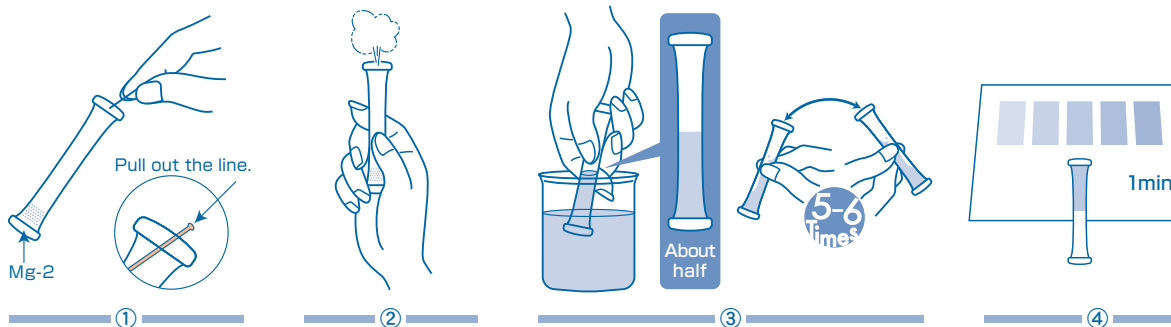

- ① Remove the colored line at the top of the tube to clear the aperture.
- ② Press the tube's side wall to expel the air, and hold the tube.

- ③ Immerse the aperture of the tube into the sample, release the finger to fill the tube halfway. Invert the tube back and forth lightly for 5 to 6 times.
- ④ Compare the actual color in the tube with Standard Color after 1 min.

How to Read the Result

At the reaction time, compare the color of the tube with Standard Color. The nearest color indicates the concentration value of the analyte in your sample. A color between two standard colors indicates the value between them.

Handling of PACKTEST Before and After Use

The content of the tube is **Strong Alkali**. Hazardous when contacting with eyes.

First Aid **Eye contact** → Immediately flush eyes with water for at least 15 minutes, followed by consult with Ophthalmologist, even without any symptom.

Skin contact → Immediately flush contacted area with water.

Ingestion → Immediately rinse mouth.

If swallowed the content or any symptom appears, seek medical advice immediately. Please refer to SDS for further information.

Storage Use PACKTEST tubes as soon as possible after opening the laminated package.

Disposal For business use, please follow in a manner consistent with relevant laws and regulations. Otherwise, the tube can be disposed as combustible waste.



KYORITSU
CHEMICAL-CHECK Lab., Corp.

1-18-2 Hakusan, Midori-ku, Yokohama, Kanagawa
226-0006, JAPAN E-mail:eng@kyoritsu-lab.co.jp

Caution

1. This product allows to measure Magnesium ion (Mg^{2+}) in the sample. If the value including turbidity, such as hydroxide, is required, please dissolve them prior to use.
2. If you need a value for magnesium hardness (the amount of magnesium converted to the equivalent of calcium carbonate), read the value at the bottom of the Standard Color.
Alternatively, multiply the measured value of magnesium ion by 4.1 to obtain Magnesium Hardness.
Magnesium Hardness ($CaCO_3$ mg/L) = Magnesium Ion (Mg mg/L) \times 4.1
3. The optimum pH upon reaction will be around 13. If the pH of the sample is below 6, please neutralize with diluted sodium hydroxide solution prior to measurement.
4. Magnesium standard solution of 30 mg/L develops color equal to or higher than 20 on Standard Color, but color development becomes weaker at 100mg/L. When the value is expected to be high, please dilute the sample prior to use.
5. Keep the sample temperature between 15-40°C. If the sample temperature is low, it requires longer reaction time.
6. Ensure that the PACKTEST tube is filled up to half. When the sample is too much, color development will be weak and it takes much longer reaction time if not enough sample volume.
7. Partially undissolved reagent will not affect the measurement.
8. When comparing to the Standard Color, please be sure to read under the daylight. It may be difficult to determine the color under the direct sunlight, certain florescent lights, mercury lamp or LED.
9. You can put the line back into the aperture to seal. This will avoid possibility of spilling the content of the tube.

Interference

Standard Color is prepared based on the standard solution. If there are some coexisting substances that may cause interference, please compare the result with official method or standard addition method for verification. Below is the list of interference data for acceptable level by adding each of the single substances to the standard solution.

- ≤ 1000 mg/L : Cl^- , K^+ , Na^+ , NH_4^+ , NO_2^- , NO_3^- , SO_4^{2-}
- ≤ 100 mg/L : Ca^{2+} , PO_4^{3-}
- ≤ 5 mg/L : Mn^{2+} , Residual Chlorine
- ≤ 1 mg/L : Cu^{2+} , Fe^{2+} , Fe^{3+} , Zn^{2+}

If interfering ions are not contained, the color will start to fade gradually after 1 minute of the reaction time. When a small amount of metal ions is contained, it takes about 5 to 10 minutes for color development.

【Caution】

- This product is made for analyzing water quality purpose only. Do not use for any other purpose.
 - This product contains small amount of chemicals. Please read instruction manual, GHS labels, SDS, and other necessary document thoroughly prior to use.
 - Please keep this information handy for future reference.
- <Safety>
- Please wash your hands thoroughly before and after the test. Do not inhale the chemical reagents.
 - It is highly recommended to wear protective gloves, eye protection, and mask upon using this product.
 - Avoid release chemical reagents or waste solution to the environment.
- <Storage>
- Please keep this product out of reach of children. Keep it in the dry and dark place at room temperature.
- <Other>
- Please check the expiration date shown on the box, and make sure to use within the date.
 - Specifications are subject to change without notice.



KYORITSU
CHEMICAL-CHECK Lab., Corp.

1-18-2 Hakusan, Midori-ku, Yokohama, Kanagawa
226-0006, JAPAN E-mail:eng@kyoritsu-lab.co.jp

2102